


60MEA2100-SG

60MEA-Signal Generator for MEA2100-(2x)60-Systems

Contact pad is disconnected for MEA2100-(2x)60-Systems.

Please ground the 60MEA2100-SG with the provided cable.

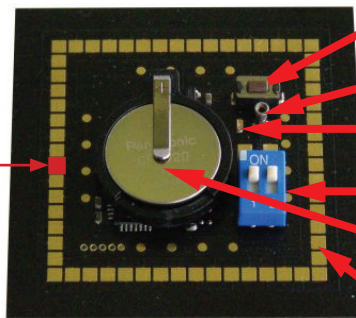

Control button

Grounding socket

LED

DIP switch

Battery

Gold contact pads

60MEA2100-Signal Generator is a very convenient tool for MEA-System users. Use the 60MEA2100-SG instead of setting up a complete experiment for training, controlling, and troubleshooting purposes.

Important: When using a 60MEA2100-SG within the MEA2100-60- or the MEA2100-2x60-System, the contact pad to the internal reference is disconnected. Otherwise the delivered signals are not acceptable. Please insert the 60MEA2100-SG in correct orientation as shown on the picture.

Switch on: Press control button. **Switch off:** Press control button longer than two seconds.

The position of DIP switch 1 and DIP switch 2 define the category of the signal, sine waves or real signals in digitized form. To change signals within one category, press the control button so many times (n) - one press slowly after the other - which are needed to create the desired signal of that category.








Please consider the different levels of amplitudes in electrode displays in direct vicinity regarding to the contact pads of 60MEA2100-SG, but not to the electrode displays. The amplitude alternates in a range of 100 % and 50 %. If there is a short circuit between neighbor pads of contact pads, all electrodes will show the same averaged amplitude. For more information, please read the MEA-Signal Generator Manual.

Table: DIP switch position, number of control button presses and corresponding signals

Switch 1	Switch 2	Control button presses n times	Signal
OFF	OFF	1 = MEA-SG ON 2 3 4 5	Sinus 0.005 Hz Sinus 0.01 Hz Sinus 0.03 Hz Sinus 1.25 Hz Sinus 12.5 Hz
ON	OFF	1 = MEA-SG ON 2 3	EPSP Population Spike Spikes
OFF	ON	1 = MEA-SG ON 2 3	ECG Atrium ECG Ventricle Ventricle FP
ON	ON	1 = MEA-SG ON	ERG with Spikes

60MEA2100-SG

60MEA-Signal Generator for MEA2100-(2x)60-Systems

Switch 1	Switch 2	Press Button slowly n times	Signal Source	Signal Type
OFF	OFF	1 The MEA-SG is on	Artificial sine waves (1.75 mV) 0.005 Hz Note: Sine waves < 1 Hz might not be visible because of the hardware filter bandwidth.	
		2	Sine wave 0.01 Hz	
		3	Sine wave 0.03 Hz	
		4	Sine wave 1.23 Hz	
		5	Sine wave 12.5 Hz	
ON	OFF	1 The MEA-SG is on	Hippocampal slice EPSP	
		2	Hippocampal slice Population spikes	
		3	Hippocampal neurons Spikes	
OFF	ON	1 The MEA-SG is on	Heart ECG Atrium	
		2	Heart ECG Ventricle	
		3	Cardiomyocytes Ventricle FP	
ON	ON	1 The MEA-SG is on	Retina ERG with spike	